



PEARL

Hospital surface disinfection using ultraviolet germicidal irradiation technology: A review

Scott, Robert; Joshi, Lovleen Tina; McGinn, Conor

Published in:

Healthcare Technology Letters

DOI:

[10.1049/htl2.12032](https://doi.org/10.1049/htl2.12032)

Publication date:

2022

Link:

[Link to publication in PEARL](#)

Citation for published version (APA):

Scott, R., Joshi, L. T., & McGinn, C. (2022). Hospital surface disinfection using ultraviolet germicidal irradiation technology: A review. *Healthcare Technology Letters*, 0(0). <https://doi.org/10.1049/htl2.12032>

All content in PEARL is protected by copyright law. Author manuscripts are made available in accordance with publisher policies. Wherever possible please cite the published version using the details provided on the item record or document. In the absence of an open licence (e.g. Creative Commons), permissions for further reuse of content should be sought from the publisher or author.

Title:	Hospital surface disinfection using ultraviolet germicidal irradiation technology: A review
Running Title:	Review of UVGI for surface disinfection
Authors	Robert Scott ¹ , Conor McGinn ^{1,2}
Institutional Affiliation	¹ Centre for Biomedical Engineering, Trinity College Dublin, Dublin, Ireland ² Akara Robotics, Dublin, Ireland
Acknowledgements	Funding for the project was provided for a grant from Science Foundation Ireland (SFI), as part of their COVID-19 Rapid Response Initiative (grant ID: 20/COV/0021).
Data Availability	The data that support the findings of this study are available from the corresponding author upon reasonable request.
Conflict of Interest	Conor McGinn declares a conflict of interest due to his involvement as a shareholder and co-founder of Akara Robotics, a company involved in the development of UVGI technology.
Ethics Approval	N/A
Patient consent statement	N/A
Permission to reproduce material from other sources	Copyright permission is obtained for using the photo in Figure 1. Images used in Figure 3 are reproducible under fair use.
Clinical trial registration	N/A

HOSPITAL SURFACE DISINFECTION USING ULTRAVIOLET GERMICIDAL IRRADIATION TECHNOLOGY: A REVIEW

PREPARED FOR HEALTHCARE TECHNOLOGY LETTERS

Robert Scott

School of Engineering
Trinity College Dublin, Ireland

Lovleen Tina Joshi

School of Biomedical Sciences
University of Plymouth, UK

Conor McGinn*

Trinity Centre for Biomedical Engineering
Trinity College Dublin, Ireland
c.mcginntcd.ie

October 29, 2021

ABSTRACT

Ultraviolet germicidal irradiation (UVGI) technologies have emerged as a promising alternative to biocides a means of surface disinfection in hospitals and other healthcare settings. This paper reviews the methods used by researchers and clinicians in deploying and evaluating the efficacy of UVGI technology. We investigated the type of UVGI technology used, the clinical setting where the device was deployed, and the methods of environmental testing that the researchers followed. Our findings suggest that clinical UVGI deployments have been growing steadily since 2010 and have increased dramatically since the start of the COVID-19 pandemic. Hardware platforms and operating procedures vary considerably between studies. Most studies measure efficacy of the technology based on the objective measurement of bacterial bioburden reduction, however studies conducted over longer durations have examined the impact of UVGI on the reduction of healthcare associated infections (HCAIs). Future trends include increased automation and the use of UVGI technologies that are safer for use around people. Although existing evidence seems to support the efficacy of UVGI as a tool capable of reducing HCAIs, more research is needed to measure the magnitude of these effects and to establish recommended best practices.

Keywords medical robotics · health hazards · man-machine systems · portable instruments

1 Introduction

Ultraviolet germicidal irradiation (UVGI) is defined as the use of ultraviolet (UV) light in the germicidal range (wavelengths: 200–320 nm) for the disinfection of air and surfaces; UVGI is distinct from the non-germicidal UVA

wavelengths of black lights and suntan lamps (320–400 nm) [1]. The first scientific reports describing the germicidal properties of ultraviolet radiation can be traced back to the nineteenth century, when Downes and Blunt [2] observed that bacteria could be inactivated by direct sunlight. The first installation of UVGI in a hospital was recorded in 1936, when an overhead UV system was installed to disinfect air in operating room settings [3]. The US Center for Disease Control (CDC) first formally sanctioned UVGI use in hospitals in 2003 as a supplemental means of water and air sanitization [4]. In 2019, the CDC Guideline for Disinfection and Sterilization in Healthcare Facilities expanded the scope of UVGI to include surfaces: *“the application of UV radiation in the health-care environment (i.e., operating rooms, isolation rooms, and biologic safety cabinets) is limited to destruction of airborne organisms or inactivation of microorganisms on surfaces.”* [5].

There are currently no harmonized European or international standards for measuring the efficacy of room decontamination using UVGI technologies. The two most applicable standards are the French norm NF T72-281:2014 “Methods of airborne disinfection of surfaces” and the US norm ASTM E3135-18 “Standard Practice for Determining Antimicrobial Efficacy of Ultraviolet Germicidal Irradiation Against Microorganisms on Carriers with Simulated Soil”. Unfortunately, neither of these standards are suitable for evaluating the microbiological efficacy of mobile UV devices [6], such as that shown in Figure 1. The occupational safety requirements of UVGI is outlined in EU Directive 2006/25/EC, which provides formulae to calculate the maximum effective radiant exposure that a person can be subjected to over an 8 hour period. In the US, UVGI devices are regulated by the Environmental Protection Agency (EPA) as pesticide devices under the Federal Insecticide, Fungicide, and Rodenticide Act (FIFRA). However, unlike with chemical disinfectants, the EPA does not routinely review the safety or efficacy of UV light devices [1].



Figure 1: Example of a robotic UVGI platform being used to disinfect surfaces in a hospital.

In the absence of formal guidance on the recommended procedures for deploying UVGI technology, there is a need to establish best practice from the currently available published literature. In section 2, we describe the methodology we followed to conduct the review. Next, we segment the field based on the type of UVGI technology, the clinical setting

¹<https://www.epa.gov/sites/default/files/2020-10/documents/uvlight-complianceadvisory.pdf>

where it was deployed, and the experimental design that was followed, and provide observations on the best practices in each. Finally, we conclude by identifying the key limitations of the study and suggest directions for future research.

2 Materials and Methods

The literature search for the review was carried out in March 2021. The first step involved identifying clinical studies that used UVGI technology. Literature searches were conducted using SCOPUS, PubMed and Google Scholar. The search involved using multiple keywords using the terms ‘UV’, ‘ultraviolet’, ‘UVGI’ with qualifiers including ‘disinfection’, ‘clinical’ and ‘hospital’ in various combinations.

The review consisted of a 3-stage process. In the first stage, we undertook a broad keyword search using the keywords outlined above, which returned 134 papers. The second stage involved reading all abstracts and removing wholly non-relevant papers such as review papers [7, 8, 9], those that involved in vitro experiments or decontamination chambers [10, 11, 12], papers not published in English, such as [13], or those unavailable for download [14]. The third stage involved re-reading the abstracts and narrowing down the papers to those that appeared to consist of real-world studies involving room decontamination using UVGI devices. Papers removed at this stage included studies using light outside the UVC spectrum [15], where the UVGI device was used to disinfect water systems [16, 17], where the device comprised a closed chamber targeted primarily at specific components (such as dental moulds [18, 19] or stethoscopes [20]), rather than full room disinfection. This led to a final selection of 53 papers being chosen for study in the analysis. A frequency analysis showing the distribution of the shortlisted papers by year is given in Figure 2. It is apparent from this chart that clinical application of UVGI technology has been growing since 2010, but increased considerably since the onset of the COVID-19 pandemic, with the number of publications in 2020 far exceeding that of each of the previous three years.

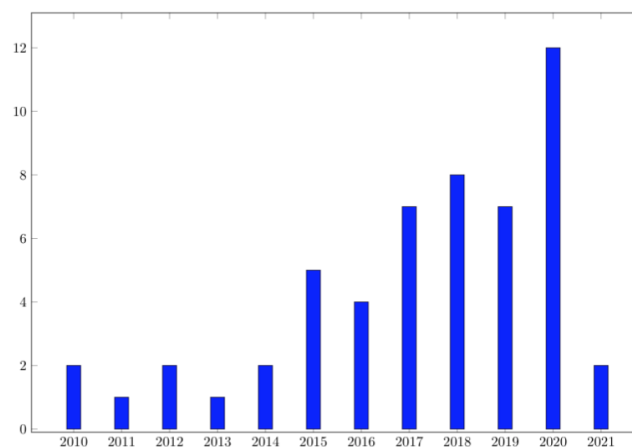


Figure 2: Distribution of clinical UVGI studies considered in our review by year (date of search 14 March 2021).

3 Results

Papers were examined under the following headings: UVGI technology, clinical settings where UVGI was used, and experimental design.

3.1 UVGI technology

For each paper reviewed, we identified the core UV-generating technology that was used (Table 1). The majority of studies (24 papers) utilized devices that produced UV irradiation using pulsed xenon (PX-UV) technology that emits broadband radiation in the 200nm-320nm spectrum. Devices using low-pressure mercury lamps (LPML), which produce narrow-band irradiation a wavelength of 254nm, were also common (20 papers). Only 2 papers investigated the efficacy of so-called Far-UV technology, which produces irradiation at 222nm using KrCl excimer lamps. UV LED's are not yet a widely used technology and were not found in the shortlisted papers in this review.

Several papers described the use of UVGI in clinical settings without describing the underlying technology that was used [21, 22, 23, 24, 25, 26] and were not included in Tables 1 or 2. While [27] utilised a UVC robot, the type of technology is unclear and was also omitted from Table 1.

Table 1: Summary of the type of UVGI technology used across the studies in the review.

Low pressure mercury lamp (LPML)	Pulsed xenon UV (PX-UV)	Far-UV
[28, 29, 30, 31, 32, 33, 34, 35, 36, 37, 38, 39, 40, 41, 42, 43, 44, 45, 46, 47]	[48, 49, 50, 51, 52, 53, 54, 55, 56, 57, 58, 59, 60, 61, 62, 63, 64, 65, 66, 67, 68, 69, 70]	[71, 72]

Next, we examined how the devices were deployed operationally during UVGI treatment. Of the devices that appeared in our review, nearly all of them were manually operated and needed to be pushed in place (41 papers) and the most widely used device was the Xenex Lightstrike (Fig. 3(a)) PX-UV system (18 papers). The second most widely used devices were the Tru-D (Fig. 3(b))(5 papers) and Skytron LPML systems (3 papers). Four papers used devices that were manually waved over the surface to be disinfected. The remaining devices were static, such as upper room fixtures (2 papers), or fully autonomous robotic devices that were able to automatically navigate to different waypoints during UVGI with minimal human intervention (1 paper). A breakdown of the degree of mobility of the devices used in each paper is given in Table 2.

3.2 Clinical settings where UVGI is used

To determine where UV disinfection has been most applicable, we examined the range of clinical settings where UVGI deployments have taken place (Table 3). It was observed that UVGI treatments were nearly always performed in rooms that did not have patients present to mitigate the risk that staff/patients might be exposed to hazardous levels of UVC irradiation during UVGI [56, 33, 69]. Patient rooms were found to be the most common location for UVGI (30 papers),

Table 2: The degree of mobility of the UVGI devices used in each study.

Fixed	Manual (push-in-place)	Manual (handheld)	Autonomous
[42, 44]	[48, 49, 28, 50, 51, 52, 53, 54, 55, 56, 30, 31, 57, 32, 33, 58, 34, 59, 60, 61, 35, 62, 63, 64, 65, 66, 37, 67, 68, 38, 39, 69, 70, 40, 27, 41, 43, 44, 45, 46, 47]	[71, 72, 36, 46]	[29]



(a)



(b)

Figure 3: Examples of UVGI devices that appear frequently in literature: (a) the Xenex LightStrike mobile device, a PX-UV device, (b) the Tru-D mobile device, a LPML device.

both for non-isolation patients and patients isolating with an infection. These settings typically consisted of a bed, a bathroom, and high touch surfaces such as bed rails, bed control panels, call button, tables, and door handles [63, 70].

Table 3: The most common clinical settings where UVGI technology was used.

Patient Rooms	ICU	OR	Other
[28, 52, 21, 53, 54, 55, 56, 71, 30, 31, 57, 32, 33, 22, 35, 62, 63, 64, 66, 37, 67, 68, 39, 69, 70, 40, 25, 43, 44, 47]	[48, 28, 55, 58, 60, 62, 36, 47]	[55, 34, 59, 60, 38, 69, 41, 42]	[49, 28, 29, 50, 51, 58, 72, 59, 60, 61, 65, 36, 23, 69, 24, 27, 45, 26, 46, 47]

Intensive care units (ICUs) and operating rooms (ORs) were the second most common setting for UVGI (8 papers each). ICUs usually consisted of patient beds, bed rails, cardiopulmonary monitors, ventilators, and other medical equipment such as keyboards and cart handles [48, 58]. Operating rooms commonly included a surgical table, anaesthetic machines and support equipment. High touch surfaces in these rooms include tray tables, monitors, infusion pumps, and scialitic lamps [55].

Other settings where the applicability of UVGI has been evaluated include burn units [69], hyperbaric chambers [27], radiology rooms [29], oncology units [35], and clinical labs within a hospital [50]. Use of UVGI technologies in hallways or other public areas was only reported in a small number of studies [28, 46]; this is likely due to challenges associated with ensuring these rooms were vacated during the UVGI procedure. Where the setting was not specifically

named [24, 26], or where various surfaces are described but the room was not named [46], the study was classified in the "Other" column of Table 3.

3.3 Experimental Design in UVGI Studies

The impact of UVGI as an infection control tool has been examined using two main approaches: (1) direct estimation of bioburden reduction, and (2) the reduction of healthcare acquired infections (HCAIs) following UVGI intervention. Based on our review, we found that the metric is generally dependent on the study duration, which is summarised in Table 4 for the papers contained in our review.

For the purpose of our analysis, short-term trials were characterised by the performance of isolated experiments, typically spanning one or several days of testing - e.g. Chen et al. [50] conducted swab sampling to compare bioburden on surfaces before and after UVGI in three rooms during a single day of testing. In total, we counted 20 short-term studies.

Medium-term studies (14 papers) were defined as periodic environmental sampling over a number of weeks or months during which a UVGI device has been in use. This generally involved more systematic testing, more closely resembling deployment within cleaning workflow - e.g. Yang et al. [32] carried out swab testing on a routine basis while the device was integrated into hospital workflow over a 6 month period between October 2015 and March 2016.

Long-term studies (18 papers) investigated the impact of UVGI devices that had been implemented into the workflow of the clinical setting for more than 12 months and/or employed HCAI reductions as the key metric. For example, Haas et al. [59] reported HCAI reductions following a 22-month deployment of a UVGI system within a contact precaution unit, operating rooms, dialysis unit and burn victim unit of an acute hospital.

Table 4: The duration of UVGI studies in the literature.

Short term	Medium term	Long term
[49, 50, 51, 56, 71]	[29, 53, 54, 55, 31]	[48, 28, 52, 21, 57]
[30, 72, 60, 63, 66, 36]	[32, 33, 58, 34, 37, 67]	[59, 61, 22, 35, 62, 64]
[38, 39, 24, 40, 27, 42]	[70, 44, 46]	[65, 68, 23, 69, 41, 45]
[73, 43, 26]		[47]

3.3.1 Environmental Sampling Methods

Measuring bioburden reduction was found to be the primary metric for short and medium-term trials. To empirically measure or quantify bio-burden reduction, it's necessary to sample surfaces in the room before and after UVGI. Of the studies reviewed in our analysis, common methods of surface sampling included contact plates, swabs, and sponges. Of the studies reviewed, the majority used a generic medium, such as Tryptone Soya Agar (TSA), which is targeted primarily at bacterial recovery. However, on occasion, selective agars were used to test for specific bacteria (such as *Clostridioides difficile* [55]) and specific fungi (such as *Aspergillus fumigatus* [32] and *Candida albicans* [46]). None of the studies in the review involved viral recovery, and therefore effectiveness of UVGI at inactivating viruses in clinical settings was not directly measured.

Contact Plate Method

The use of contact plates, also known as Replicate Organism Detection And Counting (RODAC) plates, was the most common method of sampling surfaces across UVGI studies (18 papers). Contact plates are suitable for flat surfaces and some curved surfaces (using what is known as a ‘roll plate’ method) [74]. Standard mediums, such as Tryptone Soya Agar (TSA) is typically poured into a plastic contact plate (approximately 5cm in diameter) and pressed flat against a surface in order for surface microorganisms to stick to the medium. Bioburden is most commonly quantified by counting the number of colony forming units (CFUs) on the plate after a period (typically 24–48 hrs) of aerobic incubation at 30–37°C [54, 60, 38].

Swab Method

Another common method of sampling involves using swabs (14 papers). Although they have been shown to be difficult to standardise [75], swabs have the benefit of manipulation around uneven surfaces. Typical sampling procedures involve the use of sterile swabs moistened with sterile saline and rolled on a discretized area on a surface e.g. 5cm x 5cm. Analysing swabs is more labour intensive than contact plate methods as it’s necessary to transfer microbes from the swabs to a cultivation medium post-sampling [76].

Other sampling methods

Sponges, another indirect sampling method, were observed in a small number of studies [49, 51, 55, 63]. Their use involved a sterile sponge moistened with saline being wiped across a surface and subsequently placed in a bag with Phosphate-buffered saline (PBS) and processed in a lab blender. The fluid undergoes processing before being poured onto agar plates and incubated overnight before analysis [77]. The recovery of microbes from the sponge can vary and this method is not as commonly applied as swab testing.

One study employed the use of UV sensitivity cards to estimate bioburden reduction [39]. This involves cross-referencing empirically recorded UV dose readings with standard lookup tables (like those found in [1]) citing the UVC inactivation levels for different microbes). While this method can be a useful indicator in optimising the positioning/route of a UV device, it’s not sufficient as a standalone metric in determining the disinfection efficacy since the efficacy of UVGI is dependent on the microbe, the material properties of substrate to which the microbe is attached [78], and a number of other parameters which may vary in real-world settings. Where possible, therefore, UV sensitivity measurements should be reserved as an adjunct to robust microbial sampling of the environment.

Table 5: Common methods associated with UVGI testing and validation.

Contact Plates	Swabs	HCAIs	Other
[48, 49, 29, 52, 54, 55, 31, 33, 58, 34, 72, 60, 66, 38, 69, 70, 27, 43]	[29, 50, 52, 53, 56, 71, 30, 32, 37, 67, 68, 27, 44, 46]	[48, 28, 57, 59, 61, 22, 35, 62, 64, 65, 68, 23, 69, 41, 45, 47]	[49, 55, 63, 36, 68, 23, 39, 69]

3.4 Correlation between HCAI prevalence and UVGI

The risk of healthcare associated infections (HCAIs) following patient discharge was cited by a number of studies as a major driver to implement novel disinfection technologies. The pathogens most commonly targeted in the UVGI literature, which have been identified as among the leading causes of HCAI fatalities [26], included methicillin-resistant *Staphylococcus aureus* (MRSA) (21 papers), vancomycin-resistant *Enterococcus* (VRE) (14 papers) and *Clostridioides difficile* (18 papers). Other pathogens of interest included *Escherichia coli* [36, 43, 44, 46], *Klebsiella pneumoniae* [50, 55, 43, 46] and *Pseudomonas aeruginosa* [50, 36, 69, 43, 44, 46]. The pathogens that were specifically targeted in UVGI studies are summarised in Table 6. This table combines studies that employ direct measurement of HCAI reductions as the key metric as well as studies that carried out environmental sampling and/or UVC level measurement.

Table 6: The most common pathogens of concern in the literature.

MRSA	VRE	<i>Clostridioides difficile</i>	Other
[48, 28, 52, 56, 71, 30, 31, 57, 32, 33, 58, 72, 59, 22, 62, 66, 36, 39, 70, 41, 43]	[49, 28, 53, 56, 71, 30, 31, 32, 33, 59, 61, 22, 62, 65]	[55, 56, 71, 30, 31, 59, 61, 22, 35, 62, 63, 64, 65, 23, 39, 69, 40, 25]	[28, 50, 55, 36, 69, 43, 44, 46]

A total of 16 papers reported the effect of UVGI on HCAI prevalence. Of these studies, 11 papers reported a reduction in HCAIs at a statistically significant level. The majority of papers in this category considered HCAI rates in their totality, rather than specific infection-causing microbes. With a focus on broad and efficient deployment across patient rooms, Schaffzin et al. [62] reported a 16% reduction in HCAI rates following the introduction of UVGI. Sampathkumar et al. [65] observed a decrease in HCAIs from 28.7 to 11.2 per 10,000 patient days - a 39% decrease in the PX-UV intervention period - however, the UVGI process added 25 minutes to the terminal cleaning process. A statistically significant reduction in both HCAI rate and hospitalisation rate was noted by Kovach et al. [68] in a 12-month UV intervention period when compared to the 36-month period pre-intervention. Kitagawa et al. [57] also reported statistically significant reductions of MRSA following PX-UV intervention. A 44% reduction of viral infection rates was reported in a 12-month study by Pavia et al. [45] while Napolitano et al. [47] observed a 34.2% reduction of HCAIs over an equivalent period. Raggi et al. [28] found a 19.2% of HCAIs of multi-drug resistant organisms (MDROs) after a 12-month UVGI intervention period when compared to the pre-intervention period; emergency department admissions were not adversely affected during this period.

A number of papers explored the correlation between *C. difficile* infections and the introduction of UVGI. Anderson et al. [22] recorded a significant reduction of up to 30% of *C. difficile* infections when terminal disinfection was enhanced with UVGI. Interestingly, no significant reduction was found when the standard protocol was enhanced with bleach, or a combination of bleach and UV. During a 52-week intervention period carried out by Pegues et al. [35], the *C. difficile* infection rate declined 25% in UV units while a rise of 16% was observed in non-UV units. The impact of UVGI on average room cleaning time and room turnaround was negligible. Miller et al. [64] implemented two interventions aimed at reducing *C. difficile* infections. The first intervention involved forming a multidisciplinary team

dedicated to reducing HCAs; this resulted in a reduction of 17% from baseline figures. The introduction of PX-UV as an adjunct to manual cleaning further reduced the transmission rates by 57%. A 20% reduction of hospital-acquired MDRO plus *C. difficile* rates was observed by Haas et al. [59] in a 22-month intervention period when compared to the 30-month pre-UV period. The impact of UVGI against MRSA prevalence was examined by Morikane et al. [48] who reported a 29% decrease following the implementation of the technology, as well as a 63% reduction of drug-resistant *Acinetobacter* acquisition.

Several studies did not measure significant reductions in HCAI following the introduction of UVGI. Brite et al. [61] reported no significant change in VRE and *C. difficile* incidence rates during a 20-month study period of a transplant unit. The authors note that this is likely caused by the compromised immune systems of transplant patients; they remain highly susceptible to HCAs despite a reduction in environmental pathogens following the introduction of UVGI. While Green et al. [69] observed reductions in environmental microorganisms, no significant reductions in HCAI rates were observed. Similarly, Goto et al. [23] observed no statistically significant difference in hospital-acquired *C. difficile* rates.

4 Discussion

Although the efficacy of UVGI disinfection has been established for a long time, examination of the published literature shows that the clinical practice of using UVGI technologies remains fragmented and rapidly evolving. Conventionally, UVGI has found greatest applicability in patient rooms, ICU, and OR settings, however, new applications have emerged in a diversity of settings from radiology to ambulances.

The specifications of UVGI devices vary significantly across the studies examined. In total, more than 17 distinct devices featured. Many of the manufacturers of these devices did not have publicly available datasheets and it was often not clear from the text whether the device was a commercially available platform, or a research platform. Most studies used either PX-UV technology (which irradiates using pulses across a wide spectrum of UV wavelengths) or LPML (which irradiates continuously across a narrow band of UVC wavelengths). The use of lower wavelength devices that irradiate at 222nm wavelengths (so called Far-UV) is also increasing. The effect of UVC wavelength on microbial inactivation is currently unexplored, especially in clinical settings. While studies such as that performed by Cadnum et al. [79] have attempted to investigate performance differences between PX-UV and LPML technologies, it is not possible to draw strong conclusions from their findings due to the major differences in operating procedures and hardware specifications of the platforms evaluated. Furthermore, while the majority of UVGI systems required manual positioning, newer platforms that can move autonomously seem to offer potential to reduce the labour requirements of using the technology.

The majority of UVGI studies have involved tests that take place over a single deployment of the technology. Where UVGI has been implemented over prolonged periods of time, it has often been linked with reductions in HCAI. However, given the many other factors that may confound these findings, there is a need for more systematic bio-burden measurement during long-term deployments and for more medium-to-long term studies to be conducted. Few studies

offer qualitative perspectives of the challenges of integrating UVGI within clinical workflows; this should also be addressed in future long-term studies.

While the disinfection efficacy was the primary focus in most studies, time efficiency was also of high importance [28, 21, 53, 54, 22, 62]. This is due to the demands for patient rooms and specialised units within the hospital, as well as a need to reduce the times taken to disinfect rooms without reducing disinfection efficacy. Raggi et al. [28] observed significant cost-savings in a US hospital following hospital-wide UVGI intervention; this was due to a reduction of excessive inpatient stays as a result of HCAs.

The papers reviewed in this article do not represent an exhaustive list, but we believe it does contain a good representative sample of the current state of the literature in UVGI. The keyword search was biased towards studies that were conducted in clinical environments may have missed studies conducted in other settings where UVGI is reported to be sometimes used (including hospitality, retail, etc.). The scope of the study was further limited to surface disinfection, and therefore practices involving the use of UVGI technology for inactivating microbes in air were not investigated.

Finally, despite a body of evidence indicating effectiveness of UVGI against a broad spectrum of pathogens, including microbes that are known to exhibit antimicrobial and biocide resistance, known limitations of UVGI, namely that obstructing objects may cause some surfaces to be shadowed and therefore not to receive the intended UVC dose, means that UVGI is most effectively used in conjunction with a biocide-based disinfection procedure carried out by human cleaning staff. Investigating approaches for optimizing the combined use of biocide and UVGI disinfection regimes appears to be an interesting direction for future research.

5 Conclusions

Ultraviolet germicidal irradiation has been an established means of surface and air disinfection for decades and its applications in clinical settings have been growing steadily in recent years. In this paper, we reviewed the published literature that investigated the deployment of UVGI systems in clinical systems as a means of surface disinfection. We shortlisted 52 papers in total, which were subsequently examined based on the type of UVGI technology used, the clinical settings where they were used and the experimental design that was followed in the study.

PX-UV and LP-UV technology was well represented in the literature, however, often important technical information on the devices' specifications was not publicly available. The integration of autonomous mobility and the use of far-UV as the UVGI source emerged as high potential technologies, but are currently underrepresented.

The application of UVGI room disinfection systems was limited to settings that could be evacuated during use, since high levels of background UV radiation produced by currently available UVGI devices poses a health and safety risk. Consequently, the technology has found greatest application in individual rooms after patient discharge and in operating room settings as supplementary part of routine disinfection procedures.

The majority of studies were conducted over relatively short time frames and included the empirical measurement of bioburden using standard environmental sampling techniques, whereas long term studies typically utilized HCAI prevalence measured over several months/years as the primary metric. Most of these studies indicated that the introduction of UVGI led to a measurable reduction of HCAs, however lack of standardisation and the presence of confounding factors necessitates that further studies are required before strong conclusions can be drawn.

6 Acknowledgements

Funding for the project was provided for a grant from Science Foundation Ireland (SFI), as part of their COVID-19 Rapid Response Initiative (grant ID: 20/COV/0021).

References

- [1] Wladyslaw Kowalski. *Ultraviolet germicidal irradiation handbook: UVGI for air and surface disinfection*. Springer science & business media, 2010.
- [2] Arthur Downes and T.P. Blunt. The influence of light upon the development of bacteria. *Nature*, 16(218), 1877.
- [3] Deryl Hart. Sterilization of the air in the operating room by special bactericidal radiant energy: results of its use in extrapleural thoracoplasties. *Journal of Thoracic Surgery*, 6(1):45–81, 1936.
- [4] Raymond YW Chinn and Lynne Schulster. Guidelines for environmental infection control in health-care facilities; recommendations of cdc and healthcare infection control practices advisory committee (hicpac). 2003.
- [5] William Anthony Rutala and David Jay Weber. Guideline for disinfection and sterilization in healthcare facilities (updated 2019). 2008.
- [6] John M Boyce and Curtis J Donskey. Understanding ultraviolet light surface decontamination in hospital rooms: A primer. *Infection Control & Hospital Epidemiology*, 40(9):1030–1035, 2019.
- [7] Anne C Eischeid, Jeanette A Thurston, and Karl G Linden. Uv disinfection of adenovirus: present state of the research and future directions. *Critical Reviews in Environmental Science and Technology*, 41(15):1375–1396, 2011.
- [8] John M Boyce. Modern technologies for improving cleaning and disinfection of environmental surfaces in hospitals. *Antimicrobial Resistance & Infection Control*, 5(1):1–10, 2016.
- [9] Magda Diab-El Schahawi, Walter Zingg, Margreet Vos, Hilary Humphreys, Lorena Lopez-Cerero, Astrid Fueszl, Jean Ralph Zahar, and Elisabeth Presterl. Ultraviolet disinfection robots to improve hospital cleaning: Real promise or just a gimmick? *Antimicrobial Resistance & Infection Control*, 10(1):1–3, 2021.
- [10] Gabriele Messina, Sandra Burgassi, Daniele Messina, Valerio Montagnani, and Gabriele Cevenini. A new uv-led device for automatic disinfection of stethoscope membranes. *American journal of infection control*, 43(10):e61–e66, 2015.

- [11] Hiroki Kitagawa, Toshihito Nomura, Tanuza Nazmul, Keitaro Omori, Norifumi Shigemoto, Takemasa Sakaguchi, and Hiroki Ohge. Effectiveness of 222-nm ultraviolet light on disinfecting sars-cov-2 surface contamination. *American journal of infection control*, 49(3):299–301, 2021.
- [12] Ginny Moore, Shanom Ali, Elaine A Cloutman-Green, Christina R Bradley, Martyn AC Wilkinson, John C Hartley, Adam P Fraise, and A Peter R Wilson. Use of uv-c radiation to disinfect non-critical patient care items: a laboratory assessment of the nanoclave cabinet. *BMC infectious diseases*, 12(1):1–9, 2012.
- [13] K Botzenhart, H Rüden, M Tolon, and Scharfenberg M von K. Clinical uses of ultraviolet light radiation. *Praktische Anasthesie, Wiederbelebung und Intensivtherapie*, 11(5):320–327, 1976.
- [14] Zubair Qureshi and Mohamed H Yassin. Role of ultraviolet (uv) disinfection in infection control and environmental cleaning. *Infectious Disorders-Drug Targets (Formerly Current Drug Targets-Infectious Disorders)*, 13(3):191–195, 2013.
- [15] Sarah E Bache, Michelle Maclean, Scott J MacGregor, John G Anderson, George Gettinby, John E Coia, and Ian Taggart. Clinical studies of the high-intensity narrow-spectrum light environmental decontamination system (hins-light eds), for continuous disinfection in the burn unit inpatient and outpatient settings. *Burns*, 38(1):69–76, 2012.
- [16] JC Kruithof, R Chr van der Leer, and WAM Hijnen. Practical experiences with uv disinfection in the netherlands. *Aqua- Journal of Water Supply: Research and Technology*, 41(2):88–94, 1992.
- [17] M Triassi, A Di Popolo, G Ribera D’Alcalà, Z Albanese, S Cuccurullo, S Montegrosso, M Crispino, Paola Borella, and R Zarrilli. Clinical and environmental distribution of legionella pneumophila in a university hospital in italy: efficacy of ultraviolet disinfection. *Journal of Hospital Infection*, 62(4):494–501, 2006.
- [18] Sharayu Vinod Nimonkar, Vikram M Belkhode, SR Godbole, Pranali Vinod Nimonkar, Trupti Dahane, and Seema Sathe. Comparative evaluation of the effect of chemical disinfectants and ultraviolet disinfection on dimensional stability of the polyvinyl siloxane impressions. *Journal of International Society of Preventive & Community Dentistry*, 9(2):152, 2019.
- [19] Himanshu Aeran, Sakshi Sharma, Varun Kumar, and Neelu Gupta. Use of clinical uv chamber to disinfect dental impressions: A comparative study. *Journal of clinical and diagnostic research: JCDR*, 9(8):ZC67, 2015.
- [20] Gabriele Messina, Giuseppe Spataro, Nicola Nante, Daniele Rosadini, Marco Tani, and Gabriele Cevenini. Clinical testing of a wearable automatic uv-c device for stethoscope disinfection. *American Journal of Infection Control*, 45(6):S96, 2017.
- [21] Deverick J Anderson, Lauren P Knelson, Rebekah W Moehring, Sarah S Lewis, David J Weber, Luke F Chen, Patricia F Triplett, Michael Blocker, R Marty Cooney, J Conrad Schwab, et al. Implementation lessons learned from the benefits of enhanced terminal room (betr) disinfection study: process and perceptions of enhanced disinfection with ultraviolet disinfection devices. *Infection control and hospital epidemiology*, 39(2):157, 2018.

- [22] Deverick J Anderson, Luke F Chen, David J Weber, Rebekah W Moehring, Sarah S Lewis, Patricia F Triplett, Michael Blocker, Paul Becherer, J Conrad Schwab, Lauren P Knelson, et al. Enhanced terminal room disinfection and acquisition and infection caused by multidrug-resistant organisms and clostridium difficile (the benefits of enhanced terminal room disinfection study): a cluster-randomised, multicentre, crossover study. *The Lancet*, 389(10071):805–814, 2017.
- [23] Michihiko Goto, Erin Balkenende, Gosia Clore, Rajeshwari Nair, Loretta Simbartl, Martin Evans, Nasia Safdar, Eli Perencevich, et al. Effectiveness of ultraviolet-c room disinfection on preventing healthcare-associated clostridioides difficile infection. *Infection Control & Hospital Epidemiology*, 41(S1):s33–s33, 2020.
- [24] Maureen Spencer, Michelle Vignari, Elizabeth Bryce, Helen Boehm Johnson, Loretta Fauerbach, and Denise Graham. A model for choosing an automated ultraviolet-c disinfection system and building a case for the c-suite: two case reports. *American journal of infection control*, 45(3):288–292, 2017.
- [25] Aaron N Dunn, Pavel Vaisberg, Thomas G Fraser, Curtis J Donskey, and Abhishek Deshpande. Perceptions of patients, health care workers, and environmental services staff regarding ultraviolet light room decontamination devices. *American journal of infection control*, 47(11):1290–1293, 2019.
- [26] D. L. Poster, C. C. Miller, Y. Obeng, M. T. Postek, T. E. Cowan, and R. A. Martinello. Innovative approaches to combat healthcare-associated infections using efficacy standards developed through industry and federal collaboration. 10730, 2018. Cited By :1.
- [27] Katrina Browne, Danielle Wood, Kate Clezy, Jan Lehm, and William R Walsh. Reduction of bacterial load with the addition of ultraviolet-c disinfection inside the hyperbaric chamber. *Diving and Hyperbaric Medicine*, 50(4):332–337, 2020.
- [28] Robert Raggi, Kenneth Archulet, Cody W Haag, and Weiming Tang. Clinical, operational, and financial impact of an ultraviolet-c terminal disinfection intervention at a community hospital. *American journal of infection control*, 46(11):1224–1229, 2018.
- [29] Conor McGinn, Robert Scott, Niamh Donnelly, Kim L Roberts, Marina Bogue, Christine Kiernan, and Michael Beckett. Exploring the applicability of robot-assisted uv disinfection in radiology. *Frontiers in Robotics and AI*, 7, 2020.
- [30] Michelle M Nerandzic, Jennifer L Cadnum, Michael J Pultz, and Curtis J Donskey. Evaluation of an automated ultraviolet radiation device for decontamination of clostridium difficile and other healthcare-associated pathogens in hospital rooms. *BMC infectious diseases*, 10(1):1–8, 2010.
- [31] Titus Wong, Tracey Woznow, Mike Petrie, Elena Murzello, Allison Muniak, Amin Kadora, and Elizabeth Bryce. Postdischarge decontamination of mrsa, vre, and clostridium difficile isolation rooms using 2 commercially available automated ultraviolet-c-emitting devices. *American journal of infection control*, 44(4):416–420, 2016.

- [32] Jui-Hsuan Yang, Un-In Wu, Huei-Min Tai, and Wang-Huei Sheng. Effectiveness of an ultraviolet-c disinfection system for reduction of healthcare-associated pathogens. *Journal of Microbiology, Immunology and Infection*, 52(3):487–493, 2019.
- [33] William A Rutala, Maria F Gergen, and David J Weber. Room decontamination with uv radiation. *Infection Control & Hospital Epidemiology*, 31(10):1025–1029, 2010.
- [34] Donna Armellino, Kristine Goldstein, Linti Thomas, Thomas J Walsh, and Vidmantas Petraitis. Comparative evaluation of operating room terminal cleaning by two methods: Focused multivector ultraviolet (fmuv) versus manual-chemical disinfection. *American journal of infection control*, 48(2):147–152, 2020.
- [35] David A Pegues, Jennifer Han, Cheryl Gilmar, Brooke McDonnell, and Steven Gaynes. Impact of ultraviolet germicidal irradiation for no-touch terminal room disinfection on clostridium difficile infection incidence among hematology-oncology patients. *infection control & hospital epidemiology*, 38(1):39–44, 2017.
- [36] Kazuo Umezawa, Satomi Asai, Sadaki Inokuchi, and Hayato Miyachi. A comparative study of the bactericidal activity and daily disinfection housekeeping surfaces by a new portable pulsed uv radiation device. *Current microbiology*, 64(6):581–587, 2012.
- [37] Katie Penno, Roman A Jandarov, and Madhuri M Sopirala. Effect of automated ultraviolet c–emitting device on decontamination of hospital rooms with and without real-time observation of terminal room disinfection. *American journal of infection control*, 45(11):1208–1213, 2017.
- [38] Donna Armellino, Thomas J Walsh, Vidmantas Petraitis, and Wladyslaw Kowalski. Assessment of focused multivector ultraviolet disinfection with shadowless delivery using 5-point multisided sampling of patient care equipment without manual-chemical disinfection. *American journal of infection control*, 47(4):409–414, 2019.
- [39] Vincent Masse, Michael J Hartley, Michael B Edmond, and Daniel J Diekema. Comparing and optimizing ultraviolet germicidal irradiation systems use for patient room terminal disinfection: an exploratory study using radiometry and commercial test cards. *Antimicrobial Resistance & Infection Control*, 7(1):1–7, 2018.
- [40] Andrew Zhang, Michelle M Nerandzic, Sirisha Kundrapu, and Curtis J Donskey. Does organic material on hospital surfaces reduce the effectiveness of hypochlorite and uv radiation for disinfection of clostridium difficile? *Infection Control & Hospital Epidemiology*, 34(10):1106–1108, 2013.
- [41] Sara A Ochoa, Ariadna Cruz-Córdova, Jetsi Mancilla-Rojano, Gerardo Escalona-Venegas, Veronica Esteban-Kenel, Isabel Franco-Hernández, Israel Parra-Ortega, José Arellano-Galindo, Rigoberto Hernández-Castro, Citlalli F Perez-López, et al. Control of methicillin-resistant staphylococcus aureus strains associated with a hospital outbreak involving contamination from anesthesia equipment using uv-c. *Frontiers in microbiology*, 11:3236, 2020.
- [42] Mansi U Vaidya, Gauri R Gangakhedkar, Anita N Shetty, and Pallavi V Waghalkar. A rare occurrence of accidental exposure to uv radiation among operating theatre personnel. *Indian journal of anaesthesia*, 64(3):230, 2020.

- [43] O Allen, L Jadkauskaite, NT Shafi, A Jackson, V Athithan, Y-D Chiu, IES Evans, RA Floto, and CS Haworth. Microbiological evaluation of uv disinfection effectiveness in a specialist cystic fibrosis clinic. *Journal of Cystic Fibrosis*, 18(4):e37–e39, 2019.
- [44] Y. Sedaghat, S. Gholampour, and F. T. Ghomshe. Comparison of the effectiveness of manual cleaning, hydrogen peroxidvapour and ultraviolet-c in disinfection of hospital equipment. *Infektoloski Glasnik*, 39(3):66–84, 2019. Cited By :1.
- [45] M. Pavia, E. Simpsen, M. Becker, W. K. Mainquist, and K. A. Velez. The effect of ultraviolet-c technology on viral infection incidence in a pediatric long-term care facility. *American Journal of Infection Control*, 46(6):720–722, 2018. Cited By :8.
- [46] T. Q. Corrêa, K. C. Blanco, N. M. Inada, M. D. F. Hortenci, A. A. Costa, E. D. S. Silva, P. P. Da Costa Gimenes, S. Pompeu, R. L. De Holanda E Silva, W. M. Figueiredo, and V. S. Bagnato. Manual operated ultraviolet surface decontamination for healthcare environments. *Photomedicine and Laser Surgery*, 35(12):666–671, 2017. Cited By :4.
- [47] N. A. Napolitano, T. Mahapatra, and W. Tang. The effectiveness of uv-c radiation for facility-wide environmental disinfection to reduce health care-acquired infections. *American Journal of Infection Control*, 43(12):1342–1346, 2015. Cited By :20.
- [48] Keita Morikane, Shoko Suzuki, Jun Yoshioka, Jun Yakuwa, Masaki Nakane, and Kenji Nemoto. Clinical and microbiological effect of pulsed xenon ultraviolet disinfection to reduce multidrug-resistant organisms in the intensive care unit in a japanese hospital: a before-after study. *BMC infectious diseases*, 20(1):82, 2020.
- [49] A Beal, N Mahida, K Staniforth, N Vaughan, M Clarke, and T Boswell. First uk trial of xenex px-uv, an automated ultraviolet room decontamination device in a clinical haematology and bone marrow transplantation unit. *Journal of Hospital Infection*, 93(2):164–168, 2016.
- [50] Li-hua Chen, Yu Li, Yong Qi, Shan-ni Wang, Chang-qing Gao, and Yong Wu. Evaluation of a pulsed xenon ultraviolet light device for reduction of pathogens with biofilm-forming ability and impact on environmental bioburden in clinical laboratories. *Photodiagnosis and photodynamic therapy*, 29:101544, 2020.
- [51] Jing-Jing Li, Shan-Ni Wang, Jiao-Jiao Qiao, Li-Hua Chen, Yu Li, Yong Wu, Yan-Xia Ding, Mei-Mei Wang, Yun Tian, Yun-Bo Liu, et al. Portable pulsed xenon ultraviolet light disinfection in a teaching hospital animal laboratory in china. *Journal of Photochemistry and Photobiology B: Biology*, 207:111869, 2020.
- [52] John E Zeber, Christopher Pfeiffer, John W Baddley, Jose Cadena-Zuluaga, Eileen M Stock, Laurel A Copeland, Janet Hendricks, Jwan Mohammadi, Marcos I Restrepo, and Chetan Jinadatha. Effect of pulsed xenon ultraviolet room disinfection devices on microbial counts for methicillin-resistant staphylococcus aureus and aerobic bacterial colonies. *American journal of infection control*, 46(6):668–673, 2018.

- [53] Mark Stibich, Julie Stachowiak, Benjamin Tanner, Matthew Berkheiser, Linette Moore, Issam Raad, and Roy F Chemaly. Evaluation of a pulsed-xenon ultraviolet room disinfection device for impact on hospital operations and microbial reduction. *Infection control and hospital epidemiology*, 32(3):286, 2011.
- [54] Ian Hosein, Rosie Madeloso, Wijayaratnam Nagaratnam, Frank Villamaria, Eileen Stock, and Chetan Jinadatha. Evaluation of a pulsed xenon ultraviolet light device for isolation room disinfection in a united kingdom hospital. *American journal of infection control*, 44(9):e157–e161, 2016.
- [55] Beatrice Casini, Benedetta Tuvo, Maria Luisa Cristina, Anna Maria Spagnolo, Michele Totaro, Angelo Baggiani, and Gaetano Pierpaolo Privitera. Evaluation of an ultraviolet c (uvc) light-emitting device for disinfection of high touch surfaces in hospital critical areas. *International journal of environmental research and public health*, 16(19):3572, 2019.
- [56] Michelle M Nerandzic, Priyaleela Thota, Thriveen Sankar, Annette Jencson, Jennifer L Cadnum, Amy J Ray, Robert A Salata, Richard R Watkins, and Curtis J Donskey. Evaluation of a pulsed xenon ultraviolet disinfection system for reduction of healthcare-associated pathogens in hospital rooms. *infection control & hospital epidemiology*, 36(2):192–197, 2015.
- [57] Hiroki Kitagawa, Minako Mori, Reo Kawano, Toshinori Hara, Seiya Kashiyama, Yoko Hayashi, Yayoi Sasabe, Kiyoko Ukon, Naomi Shimokawa, Toshihito Nomura, et al. Combining pulsed xenon ultraviolet disinfection with terminal manual cleaning helps reduce the acquisition rate of methicillin-resistant staphylococcus aureus. *American Journal of Infection Control*, 2021.
- [58] Hiroki Kitagawa, Minako Mori, Seiya Kashiyama, Yayoi Sasabe, Kiyoko Ukon, Naomi Shimokawa, Nobuaki Shime, and Hiroki Ohge. Effect of pulsed xenon ultraviolet disinfection on methicillin-resistant staphylococcus aureus contamination of high-touch surfaces in a japanese hospital. *American journal of infection control*, 48(2):139–142, 2020.
- [59] Janet P Haas, Jonathan Menz, Stephen Dusza, and Marisa A Montecalvo. Implementation and impact of ultraviolet environmental disinfection in an acute care setting. *American journal of infection control*, 42(6):586–590, 2014.
- [60] José E Villacís, Mario Lopez, Deborah Passey, Manuel Hernando Santillán, Germán Verdezoto, Freddy Trujillo, Gustavo Paredes, Carmen Alarcón, Ronny Horvath, and Mark Stibich. Efficacy of pulsed-xenon ultraviolet light for disinfection of high-touch surfaces in an ecuadorian hospital. *BMC infectious diseases*, 19(1):1–6, 2019.
- [61] Jennifer Brite, Tracy McMillen, Elizabeth Robilotti, Janet Sun, Hoi Yan Chow, Frederic Stell, Susan K Seo, Donna McKenna, Janet Eagan, Marisa Montecalvo, et al. Effectiveness of ultraviolet disinfection in reducing hospital-acquired clostridium difficile and vancomycin-resistant enterococcus on a bone marrow transplant unit. *Infection Control & Hospital Epidemiology*, 39(11):1301–1306, 2018.
- [62] Joshua K Schaffzin, Adam W Wilhite, Zhaoyan Li, David Finney, Andrea L Ankrum, and Ronald Moore. Maximizing efficiency in a high occupancy setting to utilize ultraviolet disinfection for isolation rooms. *American journal of infection control*, 48(8):903–909, 2020.

- [63] Shashank S Ghantaji, Mark Stibich, Julie Stachowiak, Sherry Cantu, Javier A Adachi, Issam I Raad, and Roy F Chemaly. Non-inferiority of pulsed xenon uv light versus bleach for reducing environmental clostridium difficile contamination on high-touch surfaces in clostridium difficile infection isolation rooms. *Journal of medical microbiology*, 64(Pt 2):191, 2015.
- [64] Renee Miller, Sarah Simmons, Charles Dale, Julie Stachowiak, and Mark Stibich. Utilization and impact of a pulsed-xenon ultraviolet room disinfection system and multidisciplinary care team on clostridium difficile in a long-term acute care facility. *American journal of infection control*, 43(12):1350–1353, 2015.
- [65] Priya Sampathkumar, Larry Nation, Carla Folkert, Jean E Wentink, and Kathryn W Zavaleta. A trial of pulsed xenon ultraviolet disinfection to reduce c. difficile infection. *American Journal of Infection Control*, 44(6):S32–S33, 2016.
- [66] Chetan Jinadatha, Ricardo Quezada, Thomas W Huber, Jason B Williams, John E Zeber, and Laurel A Copeland. Evaluation of a pulsed-xenon ultraviolet room disinfection device for impact on contamination levels of methicillin-resistant staphylococcus aureus. *BMC infectious diseases*, 14(1):1–7, 2014.
- [67] Hiroki Kitagawa, Minako Mori, Toshinori Hara, Seiya Kashiyama, Norifumi Shigemoto, and Hiroki Ohge. Effectiveness of pulsed xenon ultraviolet disinfection for clostridioides (clostridium) difficile surface contamination in a japanese hospital. *American Journal of Infection Control*, 49(1):55–58, 2021.
- [68] Christine R Kovach, Yavuz Taneli, Tammy Neiman, Elaine M Dyer, Alvin Jason A Arzaga, and Sheryl T Kelber. Evaluation of an ultraviolet room disinfection protocol to decrease nursing home microbial burden, infection and hospitalization rates. *BMC infectious diseases*, 17(1):1–8, 2017.
- [69] Caroline Green, Jeremy C Pamplin, Kristine N Chafin, Clinton K Murray, and Heather C Yun. Pulsed-xenon ultraviolet light disinfection in a burn unit: impact on environmental bioburden, multidrug-resistant organism acquisition and healthcare associated infections. *Burns*, 43(2):388–396, 2017.
- [70] Chetan Jinadatha, Frank C Villamaria, Marcos I Restrepo, Nagaraja Ganachari-Mallappa, I-Chia Liao, Eileen M Stock, Laurel A Copeland, and John E Zeber. Is the pulsed xenon ultraviolet light no-touch disinfection system effective on methicillin-resistant staphylococcus aureus in the absence of manual cleaning? *American journal of infection control*, 43(8):878–881, 2015.
- [71] Michelle M Nerandzic, Jennifer L Cadnum, Kevin E Eckart, and Curtis J Donskey. Evaluation of a hand-held far-ultraviolet radiation device for decontamination of clostridium difficile and other healthcare-associated pathogens. *BMC infectious diseases*, 12(1):1–6, 2012.
- [72] Yuki Kaiki, Hiroki Kitagawa, Toshinori Hara, Toshihito Nomura, Keitaro Omori, Norifumi Shigemoto, Shinya Takahashi, and Hiroki Ohge. Methicillin-resistant staphylococcus aureus contamination of hospital-use-only mobile phones and efficacy of 222-nm ultraviolet disinfection. *American Journal of Infection Control*, 2020.

- [73] Hana Hakim, Craig Gilliam, Li Tang, Jiahui Xu, and Linda D Lee. Effect of a shielded continuous ultraviolet-c air disinfection device on reduction of air and surface microbial contamination in a pediatric oncology outpatient care unit. *American journal of infection control*, 47(10):1248–1254, 2019.
- [74] Deb Reid, Karen Ternes, Linda Winowiecki, Cheryl Yonke, Brian Riege, Fabian Fregoli, Deborah Passey, Mark Stibich, and Russell N Olmsted. Germicidal irradiation of portable medical equipment: mitigating microbes and improving the margin of safety using a novel, point of care, germicidal disinfection pod. *American journal of infection control*, 48(1):103–105, 2020.
- [75] Stacey Rawlinson, Lena Ciric, and Elaine Cloutman-Green. How to carry out microbiological sampling of healthcare environment surfaces? a review of current evidence. *Journal of Hospital Infection*, 103(4):363–374, 2019.
- [76] Satu Salo, Annikki Laine, Timo Alanko, Anna-Maija Sjöberg, Gun Writanen, and Collaborators: Guðbjörnsdóttir B Jessen B Langsrud S Lindquist K Lundén J Mäki M Nerbrink E Niclasen Ó Tuominen P Tuompo H Vatunen E Woivalin A. Validation of the microbiological methods hygicult dipslide, contact plate, and swabbing in surface hygiene control: a nordic collaborative study. *Journal of AOAC International*, 83(6):1357–1366, 2000.
- [77] Kerri A Thom, Tracy Howard, Sophie Sembajwe, Anthony D Harris, Paula Strassle, Brian S Caffo, Karen C Carroll, and J Kristie Johnson. Comparison of swab and sponge methodologies for identification of acinetobacter baumannii from the hospital environment. *Journal of clinical microbiology*, 50(6):2140–2141, 2012.
- [78] Anna Gidari, Samuele Sabbatini, Sabrina Bastianelli, Sara Pierucci, Chiara Busti, Desirée Bartolini, Anna Maria Stabile, Claudia Monari, Francesco Galli, Mario Rende, et al. Sars-cov-2 survival on surfaces and the effect of uv-c light. *Viruses*, 13(3):408, 2021.
- [79] Jennifer L Cadnum, Annette L Jencson, Scott A Gestrich, Scott H Livingston, Boris A Karaman, Kevin J Benner, Brigid M Wilson, and Curtis J Donskey. A comparison of the efficacy of multiple ultraviolet light room decontamination devices in a radiology procedure room. *Infection Control & Hospital Epidemiology*, 40(2):158–163, 2019.